NOVAGEN
ANALYTICAL LABS
ADVANCED PEPTIDE TESTING SOLUTIONS

Independent Research Testing Center
875 Innovation Drive, Cambridge, MA 02139, USA

CERTIFICATE OF ANALYSIS (COA)

Product Name	Klow Blend (Injectable Research Vial)
Chemical Name	GHK-Cu / BPC-157 / TB-500 / KPV
CAS Number	89030-95-5/137525-51-0/77591-33-4/67727-97-3
Batch / Lot Number	KLOW800826
Manufacturing Date	2026-08-13
Retest / Expiry Date	2028-08-13
Net Content	80 mg total (50 mg GHK-Cu / 10 mg BPC-157 / 10 mg TB-500 / 10 mg KPV) per vial
Storage Conditions	Store at 2–8°C, protected from light and moisture
Appearance	White to off-white lyophilized powder (may have slight blue tint from copper)
Molecular Formula / MW	GHK-Cu: 402.9; BPC-157: 1419.5; TB-500: 4963.4; KPV: 342.44 g/mol

Analytical Results

Test Item	Specification	Result	Method
Identification	Conforms	Conforms	LC-MS
Purity (HPLC)	≥98.0%	98.95%	HPLC
Peptide Content	95.0–105.0%	99.4%	HPLC
Appearance	White to off-white lyophilized powder	Conforms	Visual
Water Content	≤3.0%	1.2%	Karl Fischer
Heavy Metals	≤10 ppm	<10 ppm	ICP-MS
Endotoxin	<10 EU/mg	<10 EU/mg	LAL Test

HPLC Chromatogram

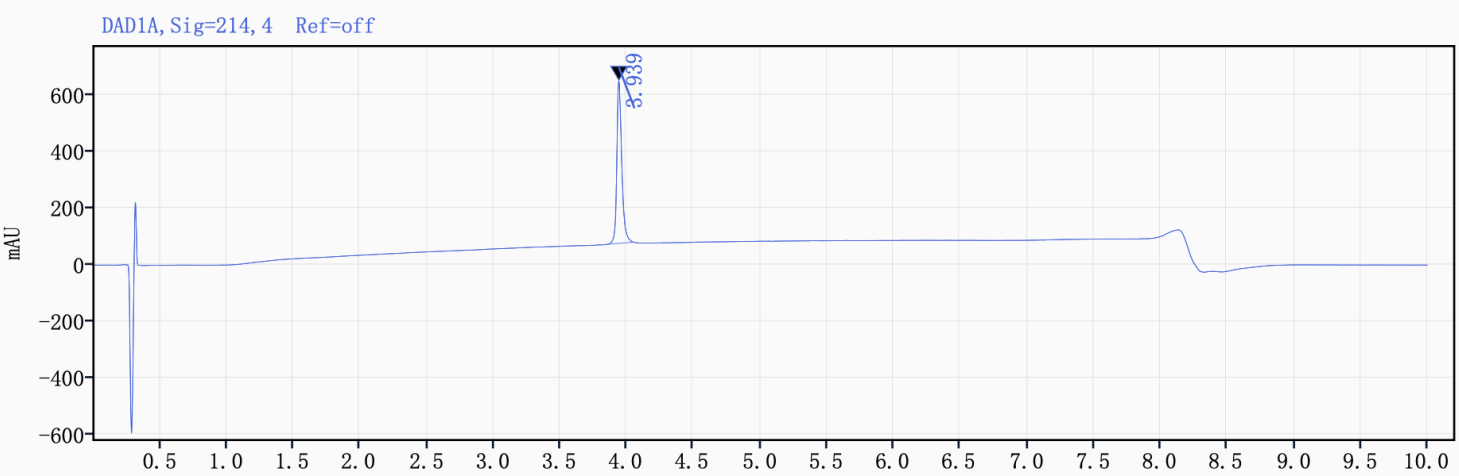

For laboratory research use only. Not for human consumption.

Tester Name	Dr. Michael Carter
Signature	Michael Carter
Test Date	2026-08-24